

Door open at setpoint -25C


Test Report Stand : 7



Item	Temperature	Minimum	Maximum	Average
1	Top left front	-25,2	-14,8	-24,1
2	Top left back	-25,6	-14,6	-24,3
3	Top right back	-25,5	-15,5	-24,4
4	Top right front	-25,6	-14,6	-24,3
5	Center	-25,5	-15,9	-24,4
6	Bottom left front	-24,2	-15,9	-23,3
7	Bottom left back	-26,4	-17,8	-25,4
8	Bottom right back	-26,1	-17,5	-25,1
9	Bottom right front	-24,6	-16,7	-23,8
10	Bottom Left	-24,5	-16,6	-23,6
11	Bottom Right	-24,5	-16,7	-23,7
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				
23				
24				

Freezers Identification	
Model	LFE 490
Serial no.	XXX
File name	LFE 490 XXX
Thermostat	-25°C
Volt / Hz	230V / 110V
Start time	15-04-2023 04:49:00
Stop time	15-04-2023 12:52:00

Comments
-25°C

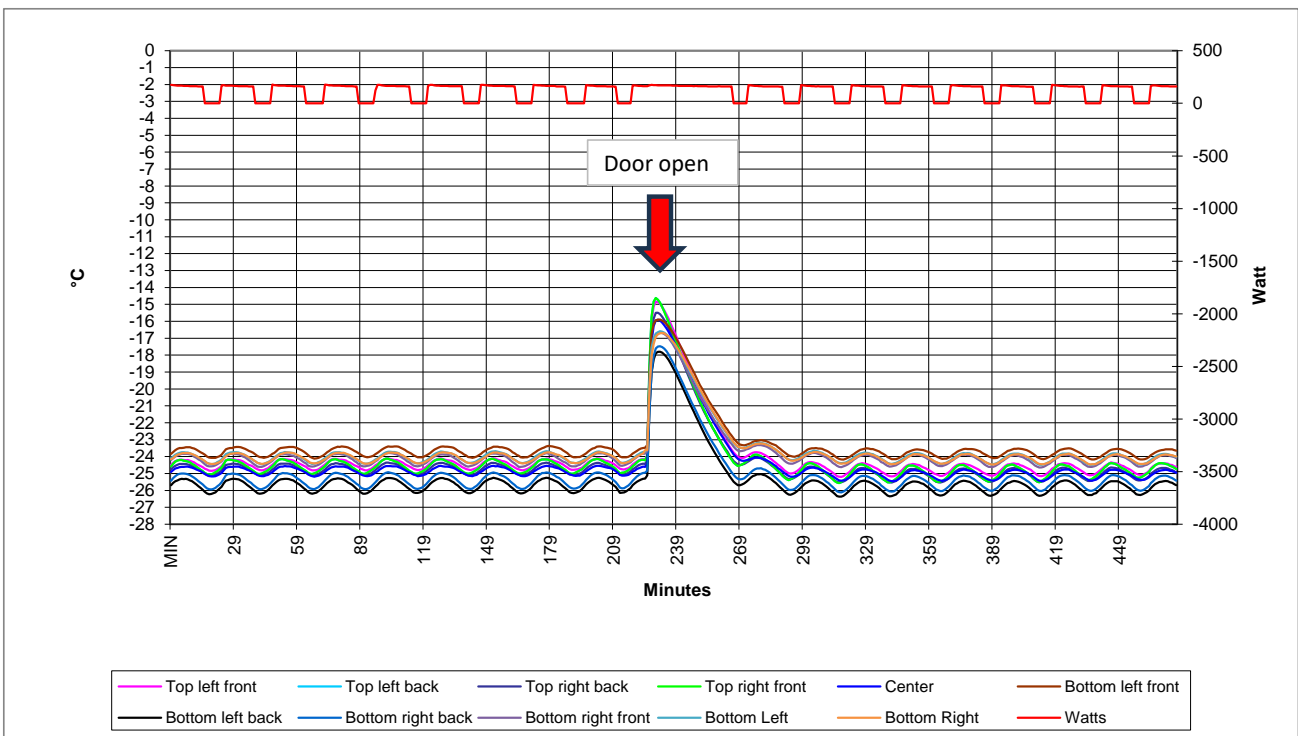

Hold over from -25C


Test Report Stand : 7



Item	Temperature	Minimum	Maximum	Average
1	Top left front	-24,8	13,7	0,8
2	Top left back	-25,0	13,7	0,9
3	Top right back	-25,0	13,7	0,9
4	Top right front	-25,0	13,7	0,9
5	Center	-25,1	13,7	0,5
6	Bottom left front	-24,0	13,8	0,8
7	Bottom left back	-26,2	13,7	0,5
8	Bottom right back	-25,9	13,8	0,5
9	Bottom right front	-24,4	13,8	0,9
10	Bottom Left	-24,2	13,8	0,9
11	Bottom Right	-24,2	13,9	0,8
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				
23				
24				

Freezers Identification	
Model	LFE 490
Serial no.	XXX
File name	LFE 490 XXX
Thermostat	-25°C
Volt / Hz	230V / 110V
Start time	16-04-2023 21:41:00
Stop time	17-04-2023 05:41:00

Comments
-25°C

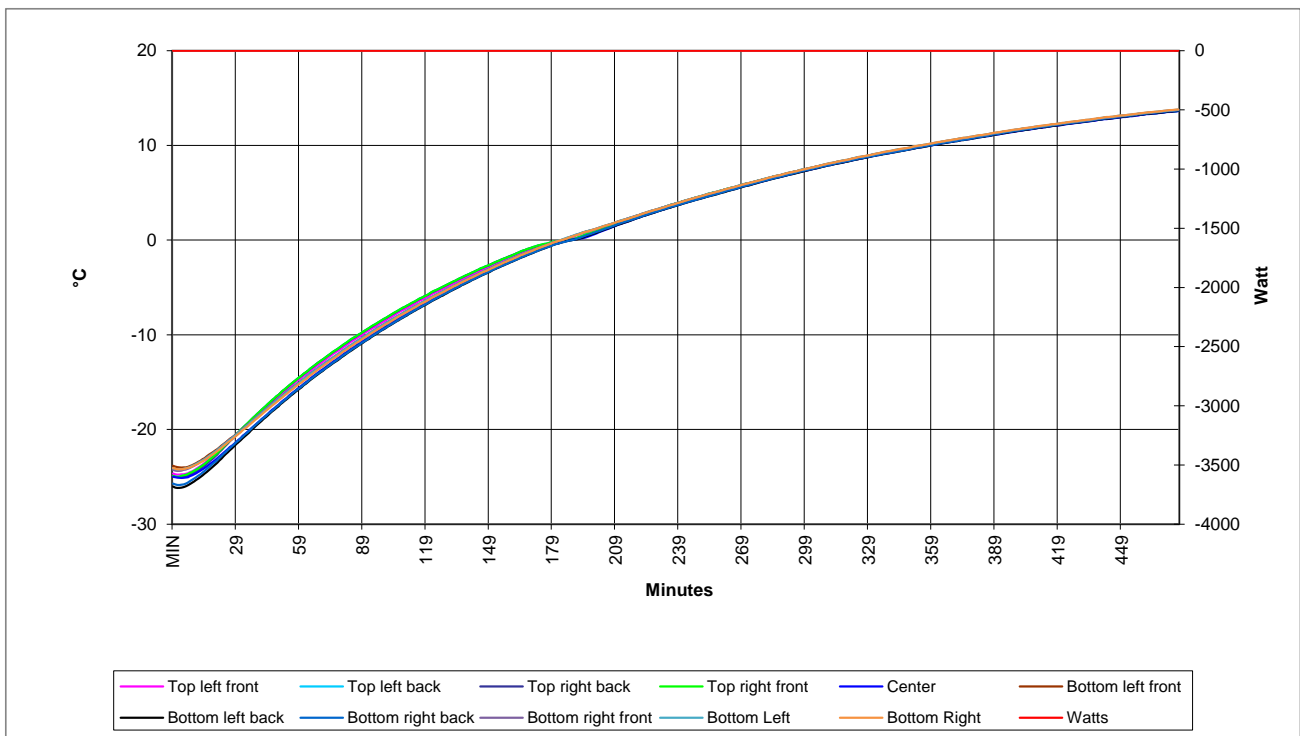

Pulldown to setpoint -25C


Test Report Stand : 7



Item	Temperature	Minimum	Maximum	Average
1	Top left front	-24,9	19,6	-20,1
2	Top left back	-25,1	20,1	-20,4
3	Top right back	-25,1	20,1	-20,4
4	Top right front	-24,9	19,6	-20,1
5	Center	-26,1	19,3	-21,4
6	Bottom left front	-24,2	19,3	-19,5
7	Bottom left back	-26,4	19,3	-21,7
8	Bottom right back	-26,1	19,3	-21,4
9	Bottom right front	-24,6	19,2	-19,9
10	Bottom Left	-24,4	19,9	-19,6
11	Bottom Right	-24,4	19,3	-19,4
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				
23				
24				

Freezers Identification	
Model	LFE 490
Serial no.	XXX
File name	LFE 490 XXX
Thermostat	-25°C
Volt / Hz	230V / 110V
Start time	14-04-2023 18:17:00
Stop time	15-04-2023 02:16:00

Comments
-25°C

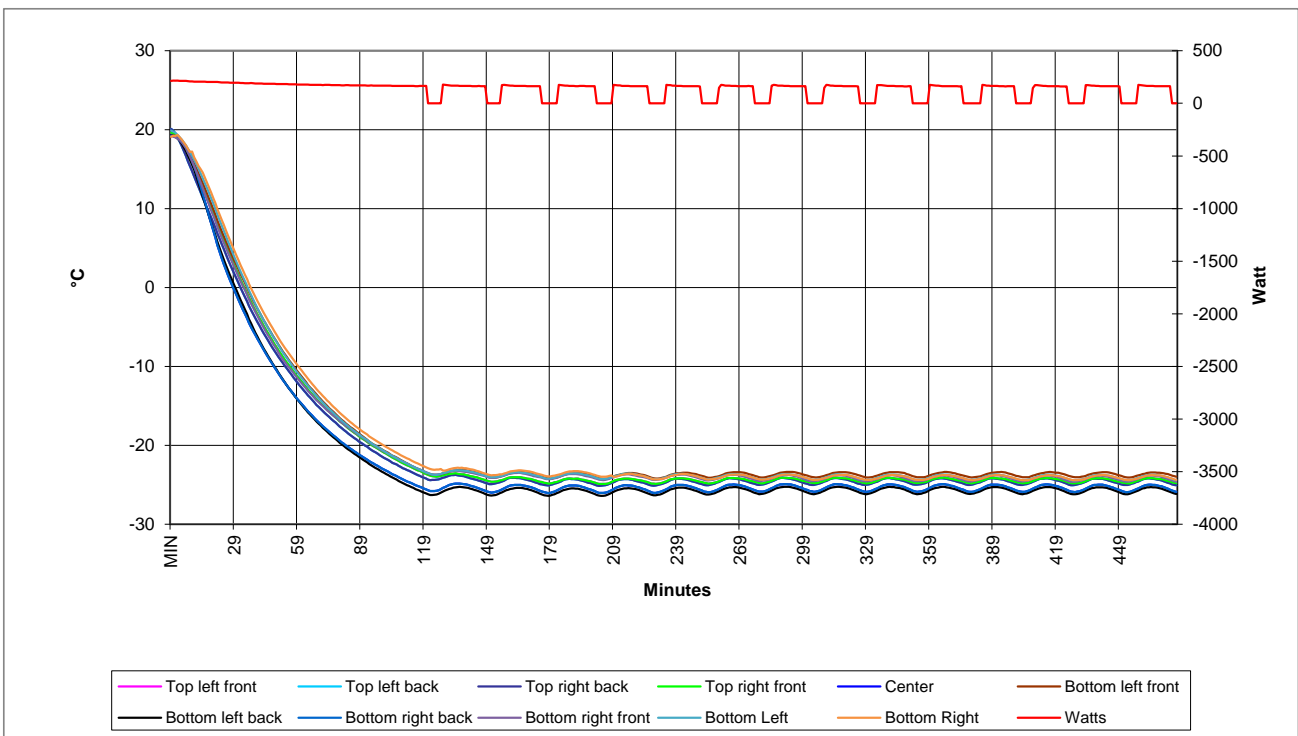

Stable at setpoint -25C

Test Report Stand : 7



Item	Temperature	Minimum	Maximum	Average
1	Top left front	-24,9	-24,1	-24,4
2	Top left back	-25,1	-24,1	-24,6
3	Top right back	-25,2	-24,4	-24,7
4	Top right front	-25,1	-24,1	-24,6
5	Center	-25,2	-24,5	-24,8
6	Bottom left front	-24,1	-23,4	-23,7
7	Bottom left back	-26,2	-25,3	-25,7
8	Bottom right back	-26,0	-24,9	-25,4
9	Bottom right front	-24,6	-23,8	-24,2
10	Bottom Left	-24,5	-23,7	-24,0
11	Bottom Right	-24,4	-23,7	-24,1
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				
23				
24				

Freezers Identification	
Model	LFE 490
Serial no.	XXX
File name	LFE 490 XXX
Thermostat	-25°C
Volt / Hz	230V / 110V
Start time	14-04-2023 23:52:00
Stop time	15-04-2023 07:52:00

**Comments**  
-25°C

